

Characterizing Ophthalmic Viscosurgical Devices (OVDs) using a rotational rheometer



RHEOLOGY AND VISCOSITY

Introduction

Ophthalmic Viscosurgical Devices (OVDs) are viscoelastic solutions or gels used to protect the corneal endothelium from mechanical trauma and to maintain intraocular space during eye surgery. They usually contain one or more of the following components; hyaluronic acid or its sodium salt, chondroitin sulfate or methylcellulose. As these materials are polymeric then they tend to be viscoelastic with their properties strongly dependent on factors such as concentration, molecular weight and molecular architecture as well as intra- or inter- molecular interactions in solution.

OVDs can be classified according to their 'cohesiveness or dispersiveness' which are ultimately related to their rheological properties. Cohesive OVDs are high viscosity materials that adhere to one another through molecular associations. They tend to have higher molecular weights and are highly shear thinning with high surface tension. Because of their high viscosity, cohesive OVDs are able to pressurize the eye and create space for insertion of the optical implant (lens). Their cohesiveness also facilitates easy removal at the end of surgery as the entire mass sticks together. In contrast dispersive OVDs tend to be lower in molecular weight and are more Newtonian. They have lower viscosities and lower surface tension making them better able to coat and adhere to both tissues and surgical instruments, and also help lubricate the optical implant during insertion. Dispersive OVDs tend to be more difficult to remove after surgery due to their higher fluidity. In addition to the two classes just described there are also combination OVDs which incorporate dispersive and cohesive properties and visco-adaptive OVDs which display different properties depending on the conditions of use.

There is now an International Standard (ISO15798:2013) detailing the requirements for characterizing these materials in terms of their biological, chemical and physical characteristics. For the purpose of this application note we are concerned with the section of the standard dealing with rheological characterisation. The standard states that the product should be tested in its finished and sterilized state at 25°C for rheological testing and involves both oscillatory and steady shear testing respectively for characterising both viscoelastic and flow characteristics in terms of the dynamic viscosity, complex viscosity and viscoelastic moduli.

The complex viscosity is measured as function oscillation frequency using logarithmic increments to simultaneously demonstrate the resistance to flow and deformation

of the OVD formulation. The frequency range specified is between 0.001 Hz and 1000 Hz but 0.01 to 100Hz is considered acceptable so long as the zero shear viscosity plateau (at diminishing frequencies) is accessible. This will occur at lower frequencies for higher viscosity materials. Often it is not possible to achieve 100Hz on a rotational rheometer due to inertial limitations and hence one should aim for the highest achievable frequency.

The elasticity or viscoelasticity of the OVD is characterised through G' and G'' and is measured simultaneously with η^* up to a frequency of 100Hz ideally, or as high as high is possible considering inertia limitations. Data should either be presented on a double logarithmic scale against frequency or as a plot of percent elasticity against log frequency, for example as $100 \times [G' / (G' + G'')] \text{ versus } \log \text{ frequency}$.

For steady shear measurements the suggested shear rate range is from 0.001 s^{-1} to approximate the zero shear viscosity, representative of conditions within the anterior chamber, to a shear rate of approximately 100 s^{-1} , to replicate conditions when the viscoelastic fluid is being injected into the eye through a cannula. The shear rates should be increased in logarithmic increments and steady shear viscosity data presented as a function of shear rate on a double logarithmic scale. Since measuring low viscosity fluids at low shear rates can be problematic then the lowest shear rate at which the zero shear viscosity can be attained is deemed acceptable. The zero shear viscosity plateau tends to appear at higher shear rates for low viscosity materials and lower shear rates for high viscosity materials so low shear rates are not always needed. Note that the steady shear zero shear viscosity should correspond with the equivalent value of η^* measured using oscillatory testing.

Experimental

- An OVD formulation containing hyaluronic acid at three different concentrations 15mg/ml, 18mg/ml and 25mg/ml was analyzed and compared according to ISO15798:2013
- Rotational rheometer measurements were made using a Kinexus rotational rheometer with a Peltier plate cartridge and using $4^\circ/40\text{mm}$ cone-plate measuring system for oscillatory measurements and a $2^\circ/20\text{mm}$ cone-plate for viscometry tests
- A standard loading sequence was used to ensure that both samples were subject to a consistent and controllable loading protocol. All rheology measurements were performed at 25°C .
- A strain controlled frequency sweep within the pre-determined linear viscoelastic was performed to determine G' , G'' and η^* as a function of frequency
- An equilibrium table of shear rates test was performed to determine the steady state shear (dynamic) viscosity as a function of shear rate
- Values of η_0 were attained by means of a Cross-model analysis within the rSpace software

Results and Discussion

Oscillation testing

The complex viscosity curves as a function of angular frequency ($\omega = 2\pi f$) are shown in Figure 1. These curves are typical of a viscoelastic fluid, where at high frequencies the complex viscosity is low (more elastic) and increases with decreasing frequency as elastic energy is converted to viscous energy, culminating in a constant viscosity plateau. The onset of this constant viscosity or zero shear viscosity plateau (η^*_0) is clearly visible for all samples with the higher concentrations having higher viscosities.

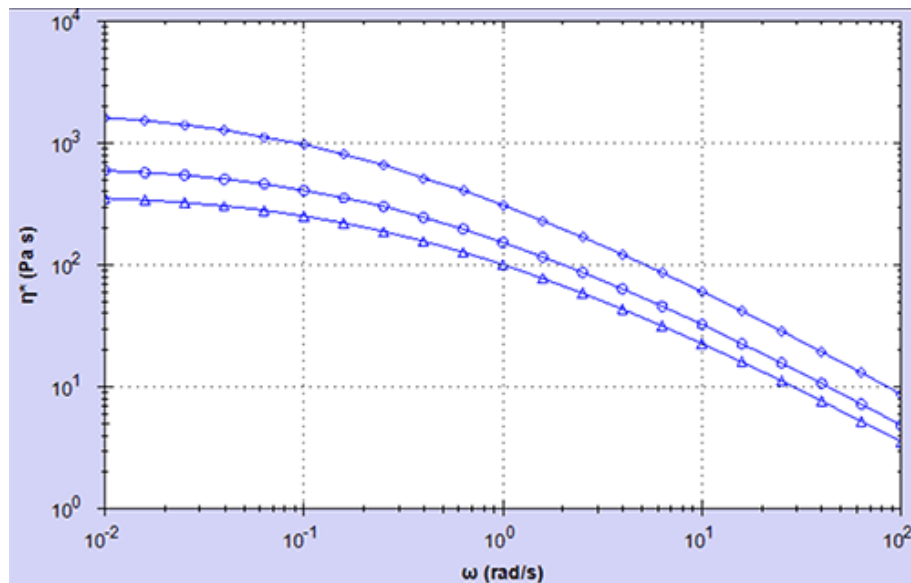


Figure 1. Frequency sweep data showing complex viscosity as a function of angular frequency for 25mg/ml (\diamond), 18mg/ml (\circ) and 15mg/ml (Δ) HA solutions

Figure 2 shows G' and G'' curves over the same frequency range for the three HA solutions. At high frequencies the elastic modulus G' is dominant, concomitant with a low value of η^* and decays with decreasing frequency (increasing time) as elastic energy is converted into viscous energy, consistent with the increase and eventual plateau in η^* .

The G'/G'' crossover indicates a transition from elastic dominant (pseudo-gel like) behavior to liquid dominant behavior with the inverse of the crossover frequency $1/\omega_c$ representing the longest relaxation time of the material or the time it takes for approx. 63% of the elastic energy or stress to be dissipated as the polymer relaxes. The modulus at this crossover point can be referred to as the 'crossover modulus' (G_c) and is a measure of the total stiffness at this angular frequency. As with η^* , the HA solutions with the highest concentrations have the largest values of G' across all frequencies and also the longest relaxation time. This is consistent with a higher number of inter-molecular interactions or entanglements making these materials behave more elastic for longer when stressed.

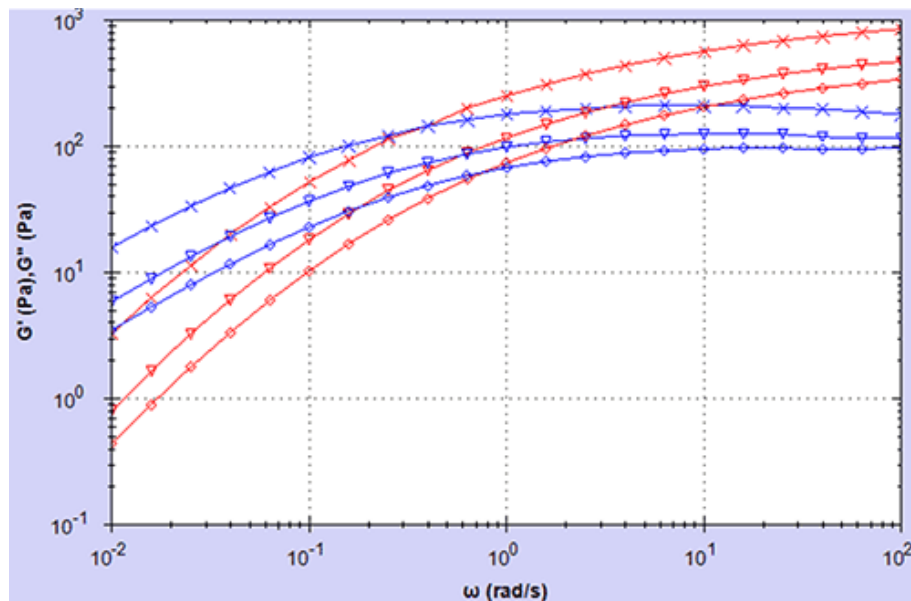


Figure 2. Frequency sweep data showing G' (red) and G'' (blue) as a function of angular frequency for 25mg/ml (x), 18mg/ml (▼) and 15mg/ml (◊) HA solutions

Viscometry testing

Steady state flow curves for the three HA solutions are shown in Figure 3. All samples are shear-thinning or pseudoplastic showing a drop in viscosity with increasing shear rate which largely mirrors the complex viscosity vs angular frequency curves in Figure 1. This is one of the reasons complex viscosity data is plotted against angular frequency, since angular frequency can be equivocated with shear rate and for simple liquid and polymeric systems $\eta^*(\omega) \approx \eta(\dot{\gamma})$ as ω tends to zero. In this case η and η^* data agree very well in the low frequency, low shear rate region with comparable values of η_0 and the same concentration trend.

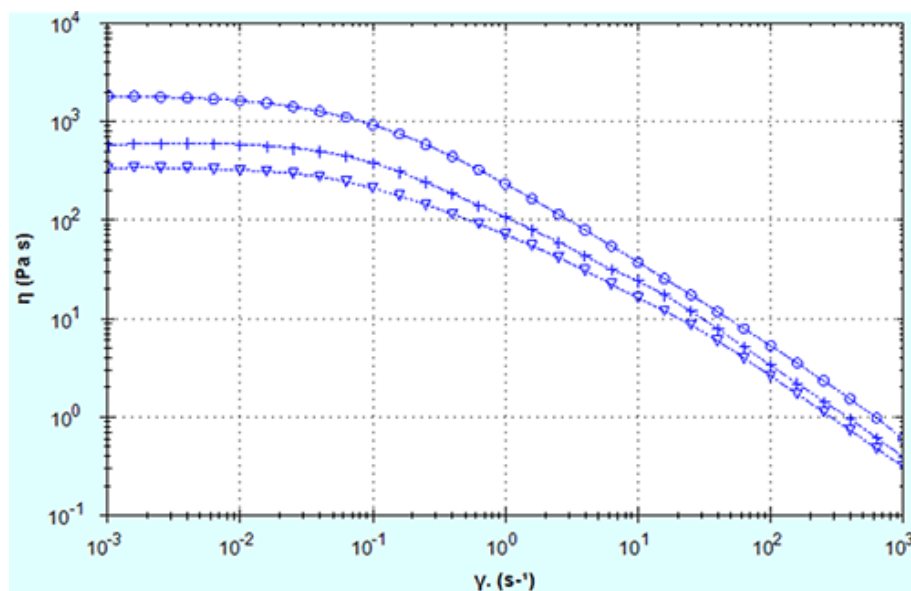


Figure 3. Equilibrium flow curve data showing dynamic viscosity as a function of shear rate for 25mg/ml (◊), 18mg/ml (+) and 15mg/ml (▼) HA solutions

Data analysis

The zero shear viscosity can be estimated directly by taking a single point or an average of multiple points within the zero shear viscosity plateau. An alternative and often preferred method is to apply a rheological model which is known to fit curves of this type very well. These models include the Cross and Carreau models which are available within the rSpace software. These can be fitted to both $\eta^*(\omega)$ and $\eta(\dot{\gamma})$ data, as long as the correlation coefficient for the fit is high. Figure 4 shows a Cross model fitted to viscosity-shear rate data for the 15mg/ml HA solution and demonstrates how well this model fits the data.

Zero shear viscosity for all samples based on cross model fitting of $\eta^*(\omega)$ and $\eta^*(\dot{\gamma})$ data are listed in Table 1. Automated crossover analysis data for G' and G'' curves are also reported.

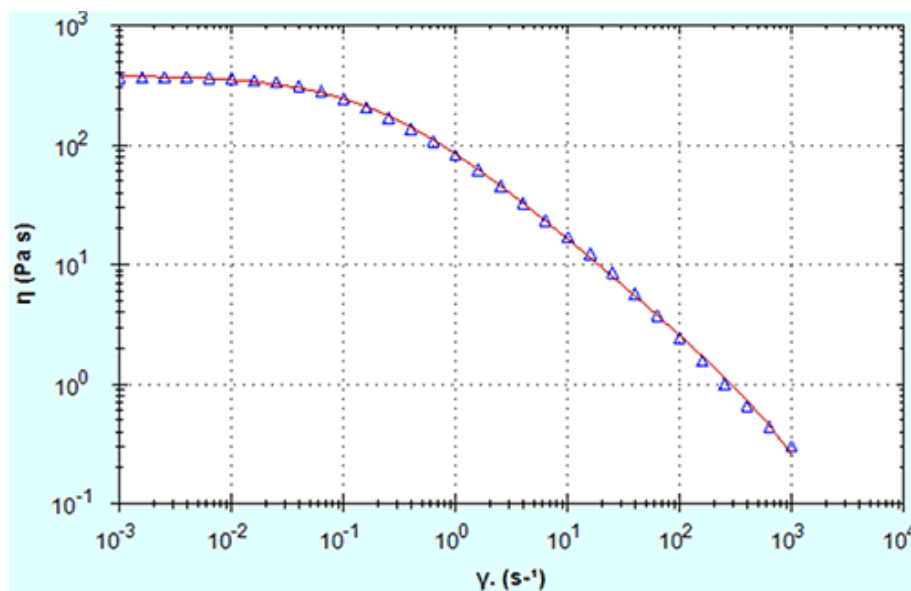


Figure 4. Equilibrium flow curve data showing dynamic viscosity as a function of shear rate for 15mg/ml HA (Δ) fitted with a Cross model (red line)

Higher values of η_0 indicate lower mobility and hence more cohesive properties while lower values indicate better dispersiveness. In terms of G' and G'' data a lower cross over frequency (ω_c) and higher crossover modulus (G_c) would indicate a more cohesive structure, while a higher value of ω_c and lower value of G_c would indicate a more dispersive system. More generally dispersive OVDs tend to have η_0 values less than 50Pas and cohesive OVDs anywhere between 100 and 100000 Pas with these higher viscosities usually associated with higher values of G_c and lower values of ω_c . According to this criteria the three solutions tested would be classified as being more cohesive than dispersive in nature.

Conclusion

The rheological properties of an HA based OVD at three different HA concentrations were evaluated according to ISO15798:2013 using a Kinexus rotational rheometer. This involved measuring the steady state dynamic shear viscosity, complex viscosity and viscoelastic moduli (G' and G''). The different samples were characterized and compared in terms of their zero shear viscosities and relaxation profiles respectively in order to better classify them in terms of their 'cohesive and dispersive' properties.

References

1. ISO 15798:2013(E) - Ophthalmic implants — Ophthalmic viscosurgical devices
2. Arshinoff, S.A. Ophthalmic viscosurgical devices. In Cataract and Refractive Surgery (Essentials in Ophthalmology Series). Springer-Verlag, Berlin, Germany; 2005:37–62
3. Webinar - "Polymer solution characterization – Part 4: Rheology and viscosity or "stretch and flow"" Malvern Instruments (download from www.malvern.com)
4. Webinar - "The validity of the Cox-Merz rule" Malvern Instruments (download from www.malvern.com)
5. Application note – Characterizing gel properties using oscillation testing on a rotational rheometer (download from www.malvern.com)



Malvern Instruments Limited
Groewood Road, Malvern,
Worcestershire, UK. WR14
1XZ

Tel: +44 1684 892456
Fax: +44 1684 892789
www.malvern.com

Malvern Instruments is part of Spectris plc, the Precision Instrumentation and Controls Company.

Spectris and the Spectris logo are Trade Marks of Spectris plc.



All information supplied within is correct at time of publication.

Malvern Instruments pursues a policy of continual improvement due to technical development. We therefore reserve the right to deviate from information, descriptions, and specifications in this publication without notice. Malvern Instruments shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance or use of this material.

Malvern Instruments owns the following registered trademarks: Bohlin, FIPA, Insitex, ISYS, Kinexus, Malvern, Malvern 'Hills' logo, Mastersizer, MicroCal, Morphologi, Rosand, 'SEC-MALS', Viscosizer, Viscotek, Viscogel and Zetasizer.